



## **CranioXpand**

Cranial springs for the treatment  
of sagittal craniosynostoses



Oral and maxillofacial surgery is our passion! Its further development, together with our customers, is our ambition. Every day we work on developing innovative products and services which meet the highest demands on quality, and which contribute to the wellbeing of the patient.

## Contents

	Pages
Introduction	4 – 5
Product features	6 – 9
Fields of use and surgical technique	10 – 24
■ Scaphocephalus due to sagittal craniosynostosis	12 – 24
Product range	26 – 31
■ Implants	26 – 27
■ Instruments	28 – 29
■ Storage	30 – 31





## **CranioXpand**

### Cranial springs for the minimally invasive treatment of sagittal craniosynostoses

The therapy of craniosynostosis is a challenging task that requires an individual treatment plan tailored to the specific characteristics of each child.

For this reason, various methods and procedures have become established in the past which can be used for surgical correction.

The use of cranial springs is considered to be a minimally invasive technique, which offers several advantages versus open treatment concepts, in particular significantly reduced blood loss as well as shorter times for surgery and thus also anesthesia. This significantly reduces stress on the young patient.

With CranioXpand – a holistic system based on the many years of experience of Dr. Noor ul Owase Jeelani – proven springs are available to support the surgeon in everyday clinical practice. In combination with a standardized surgical technique and instruments specifically designed for this purpose, supportive conditions for successful treatment are given.

## Feature, function and benefit







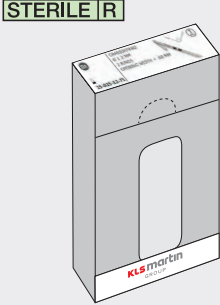
KLS Martin aims to offer a fully comprehensive portfolio of products for the surgical correction of cranial malformations, supporting tailored care approaches for the specific situation.

In addition to various cranial distractors and resorbable implants, cranial springs are now available for the minimally invasive treatment of craniosynostosis.

CranioXpand springs are designed to support a high level of protection. The rounded, atraumatic design supports smooth embedding in the soft tissue, while the angled ends are intended to promote stable anchorage and secure positioning within the bone.

CranioXpand springs are available in different wire strengths or forces and are marked accordingly for easy identification.

## CranioXpand – Implants

Feature	Benefit
	<ul style="list-style-type: none"> <li>■ Cranial springs in different wire thicknesses: <ul style="list-style-type: none"> <li>■ Wire thickness Ø 1.0 mm = 5 N</li> <li>■ Wire thickness Ø 1.2 mm = 8 N</li> <li>■ Wire thickness Ø 1.6 mm = 13 N</li> </ul> </li> <li>■ Broad product selection tailored to the type and severity of the malformation to be treated</li> <li>■ Reliable determination of the spring thickness with the selection instrument adapted to the surgical technique</li> </ul>
	<ul style="list-style-type: none"> <li>■ Identification of the springs according to the wire thickness: <ul style="list-style-type: none"> <li>■ Wire thickness Ø 1.0 mm = no ring</li> <li>■ Wire thickness Ø 1.2 mm = 2 rings</li> <li>■ Wire thickness Ø 1.6 mm = 6 rings</li> </ul> </li> <li>■ Unique identification and differentiation</li> </ul>
	<ul style="list-style-type: none"> <li>■ Angled, atraumatic ends</li> <li>■ Designed to promote stable anchorage within the bone</li> <li>■ Supports secure positioning and reliable fit of the spring</li> </ul>
	<ul style="list-style-type: none"> <li>■ Implants made of high-quality medical implant steel</li> <li>■ Provides mechanical stability</li> <li>■ Proven biocompatibility</li> </ul>
	<ul style="list-style-type: none"> <li>■ All springs are available in individually sterile packaged versions</li> <li>■ Direct, swift and application-oriented access</li> <li>■ Including self-adhesive labels with all the relevant implant data</li> <li>■ Support of aseptic handling due to double sterile packaging (primary and secondary blister)</li> <li>■ Batch-specific labeling to support traceability and clear, patient-related documentation</li> </ul>

## Feature, function and benefit



KLS Martin has set itself the goal of designing system-specific instruments that support easy and efficient handling, contributing to streamlined surgical workflows.






For this reason, the focus during development was not only on instruments perfectly matched to the surgical technique with good haptics, but also on intuitive, easy operability.

The special insertion instruments are designed to facilitate easy pick-up as well as adjustable compression of the spring, supporting controlled handling during implantation.

In addition to enabling direct access to the instruments, the storage system is designed to support efficient reprocessing, addressing the practical needs of all stakeholders involved



## CranioXpand – Instruments and Storage

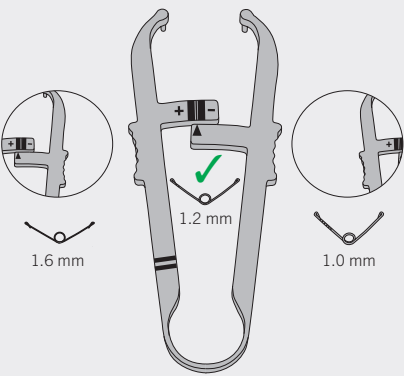Feature	Benefit
	<ul style="list-style-type: none"> <li>■ Insertion instruments specifically matched to the springs</li> <li>■ Easy pick-up of the spring</li> <li>■ Supports controlled compression and secure retention of the spring during placement</li> <li>■ Designed to support safe and flexible implantation, with the spring opening either anterior or posterior</li> </ul>
	<ul style="list-style-type: none"> <li>■ Instrument for the easy determination of the appropriate spring force</li> <li>■ Facilitates selection of the correct spring force</li> <li>■ Adapted to the proven surgical technique and to an intra-operative opening of the gap of 15 mm</li> </ul>
	<ul style="list-style-type: none"> <li>■ Stainless steel storage containers of honeycomb design combined with high-performance plastic.</li> <li>■ High strength, light weight</li> <li>■ Good rinsing capability due to large openings and reprocessing-optimized design</li> </ul>
	<ul style="list-style-type: none"> <li>■ In the storage container the instruments are arranged according to the sequence of use during surgery</li> <li>■ Swift and intuitive supply of instruments during surgery</li> <li>■ User-friendly and efficient passing of instruments to the surgeon</li> <li>■ Transparent organization and arrangement</li> </ul>
	<ul style="list-style-type: none"> <li>■ Storage locations marked with laser images and article numbers of the instruments to be stored.</li> <li>■ Facilitates sorting of the instruments into the storage container</li> <li>■ Transparent organization and arrangement</li> </ul>

## Step by step to optimal care

### Fields of use

Minimally invasive treatment of scaphocephalus due to sagittal craniosynostosis in children aged three to eight months.



Scaphocephalus  
Clinical picture



## Surgical technique

### **Scaphocephalus due to sagittal craniosynostosis**

Treatment with two cranial springs, Ø 1.2 mm

Pages 12 – 24

Dr. Noor ul Owase Jeelani





### Preoperative planning

The diagnosis of sagittal craniosynostosis caused by the premature fusion of the sagittal suture is typically made on the basis of a clinical examination. The illustration on the right shows a patient with a clinical picture typical of scaphocephaly.




### Positioning of the patient

The patient is placed face-down in the "sphinx" position on the operating table, whereby the neck is extended and the chin is placed on a horseshoe gel roll.

Support is provided at the chest and pelvis to ensure there is no abdominal compression which may impede venous return.

The head of the table is raised some 20 degrees until the top of the head is parallel with the operation room floor. Use a sandbag to ensure that the child does not slip down the table.

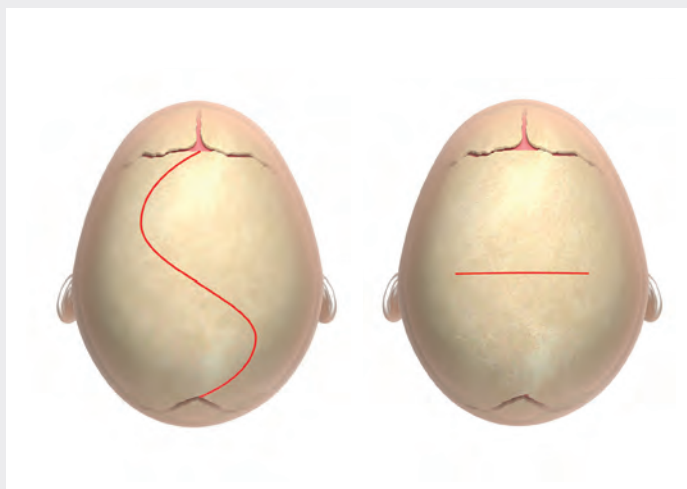

## 1. Approach


There are two options available for skin incision:

### S-shaped incision

The opening can be made via an S-shaped incision over the sagittal suture. This provides exposure from the anterior fontanelle (which may be closed) to the confluence of the lambdoid sutures to provide excellent access to the cranium. This approach is recommended to gain initial experience with the technique. However, the advantage of a better view is countered by the disadvantage of a larger scar, as well as the problem that a section of the scar lies above the springs.

### Perpendicular incision

Alternatively, an 8 cm incision can be made perpendicular to the sagittal suture. The anteroposterior location of the incision is approximately at the half way point between the anterior fontanelle and the confluence of the lambdoid sutures. The location may be adjusted depending on the expression of scaphocephaly. Two perpendicular incisions may be used for more severe cases or where the occipital protuberance may be a particular issue.

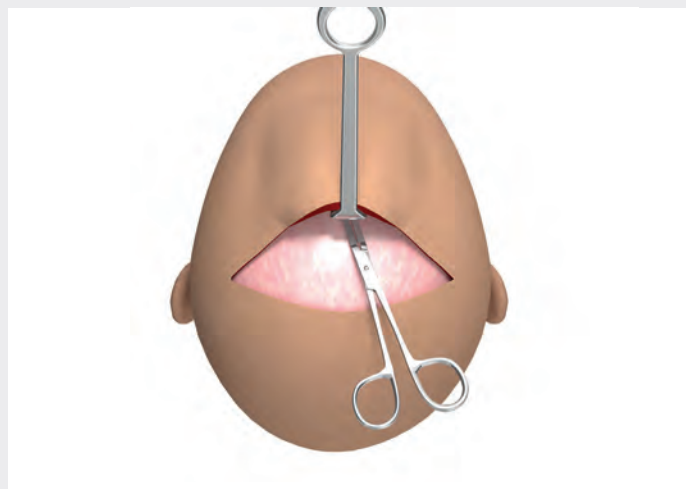


## 2. Exposure of the calvarium

After skin incision, the galea is transected to the subgaleal space. Blunt preparation with scissors and monopolar electrocautery follows in the relatively poorly perfused sub-galeal plane, exposing the calvarium from just anterior to the coronal sutures to past the lambdoid sutures. A “surgical corridor” approximately 4–5 cm wide is created in this plane.

### Note:

*As a precaution, approach and exposure should be performed separately. Any surgery employing a minimally invasive approach should allow switching to open surgery should the need arise. For the 8 cm perpendicular incision, the incision should be marked as a full bicoronal incision. The prep and drape are to be performed accordingly, so that should the need arise, the entire calvarium may be exposed. The other major advantage of prepping and draping the whole head is that it allows better orientation. With a minimal approach, internal landmarks may possibly not be easy to identify. Therefore, including the entire calvarium where the sutures are marked on the skin to begin with can prove most valuable in orienting the surgeon in the surgical field.*



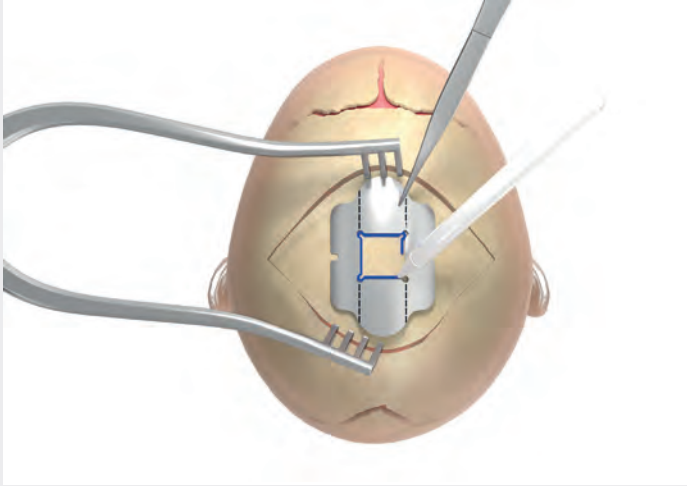

### 3. Marking the central craniectomy and parasagittal osteotomies

Open the soft tissue using wound retractors and then elevate.

To open the skull, a square piece of bone (15 mm<sup>2</sup>) is removed from the center of the calvarium (craniectomy). The marking template is used to mark the outer contour of the square as well as the positions of the four burr holes in the corners.


The anteroposterior location of the square is roughly halfway between the anterior fontanelle and the confluence of the lambdoid sutures. This position may be altered to find the narrowest point of the skull.

After outlining the marks, the template is removed.

The two parasagittal osteotomies run in extension of the lateral edges of the square and are marked appropriately up to the frontal fontanelle as well as the confluence of the lambdoid sutures. Posteriorly, near the lambdoid sutures, the parasagittal incisions may fan out.



Template for marking

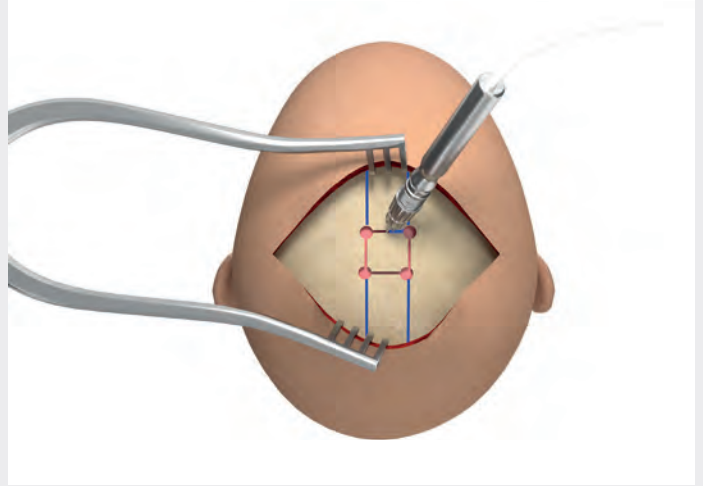


### 4. Opening of the calvarium



The drill holes are created via trepanation in the four corners of the marked square. Bone wax is filled into the holes to control bleeding, as necessary.

Once the dura is freed, the burr holes are joined using a craniotome with dura protector. The square piece of bone is then removed.

*Note:*

*Great care must be taken as the sagittal sinus often indents the fused sagittal suture and rests in a U-shaped groove on the inside of the calvarium. The craniotomy bone cuts, as per standard neurosurgical practice, should come up to the middle but not cross it.*


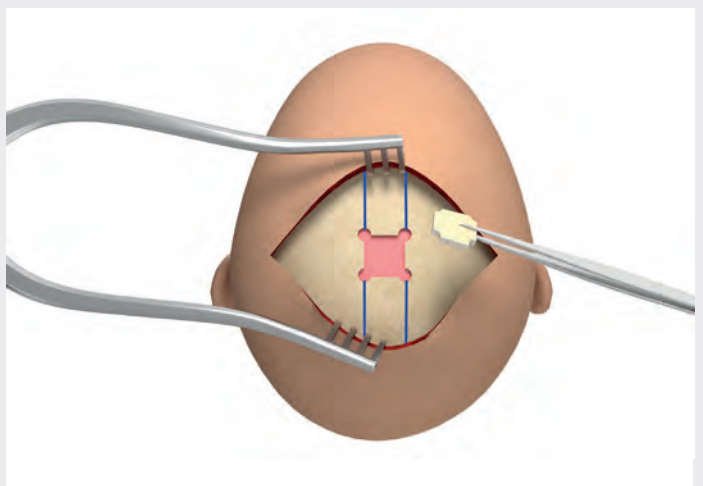


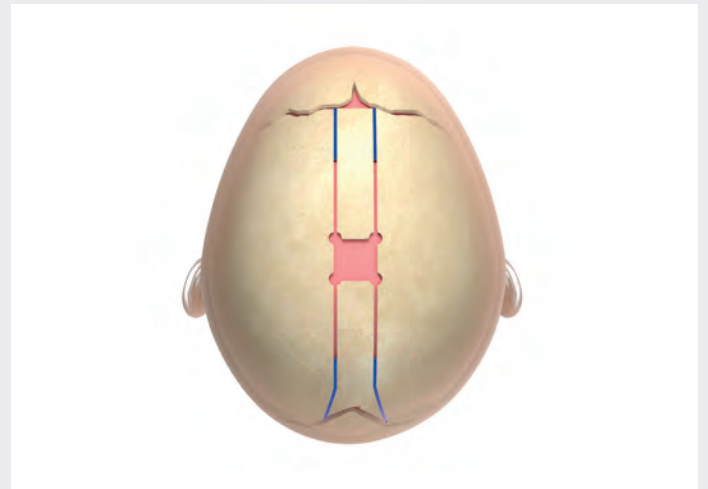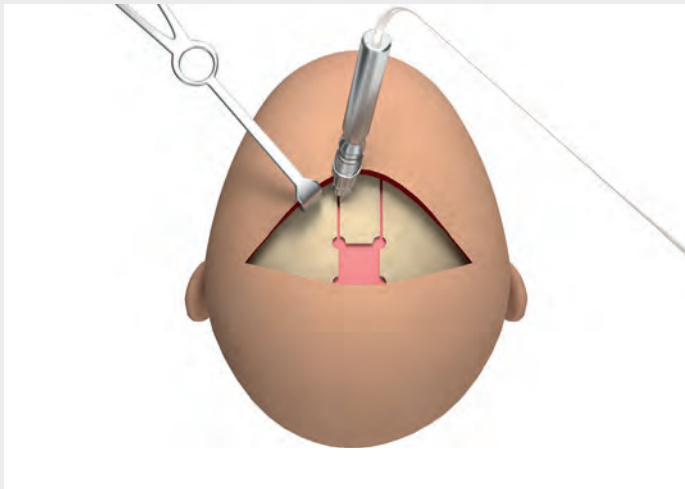

## 5. Performing the osteotomies


After removing the square of bone, the dura is stripped from the overlying calvarium under direct vision along the entire length of the planned parasagittal osteotomies. Starting from the lateral edges of the square, the two parallel osteotomies between the anterior and posterior fontanelles are performed with the craniotome and dura protector, whereby the sagittal suture lies in the middle.

Anteriorly, osteotomies may terminate in a free fontanelle or the coronal sutures. Posteriorly, the osteotomies diverge slightly in a fan shape when they bisect the lambdoid sutures. The primary aim is to keep them as far away from the sagittal suture as possible (approx. 10-15 mm). An additional bonus is that this results in the forces being more uniformly dissipated across the osteotomy-suture construct, resulting in less lambdoid ridging.

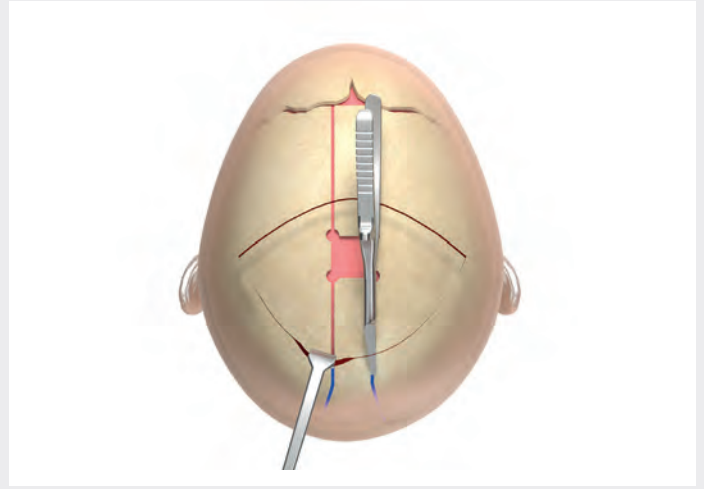
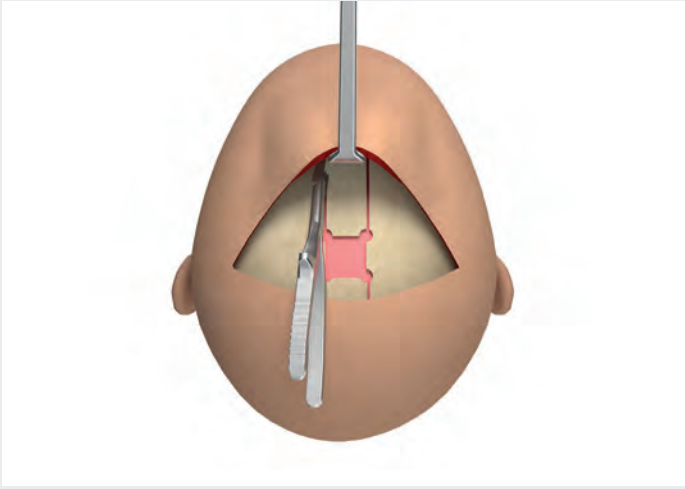


The most anterior and posterior parts of the osteotomies which are difficult to reach with the craniotome are finalized using the bone cutting forceps. In doing this, a midline strip is generated.

It is possible that diploid veins may be encountered in the middle line. These are coagulated using bipolar cautery under direct vision. At the end of this step, the anterior and posterior sagittal struts should be hinged quite freely on the coronal and lambdoid sutures. If this is not the case, the surgeon should ascertain that the parasagittal cuts are indeed complete and the dura stripped free.

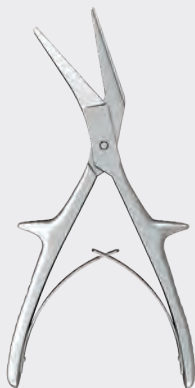

Bone cutting forceps

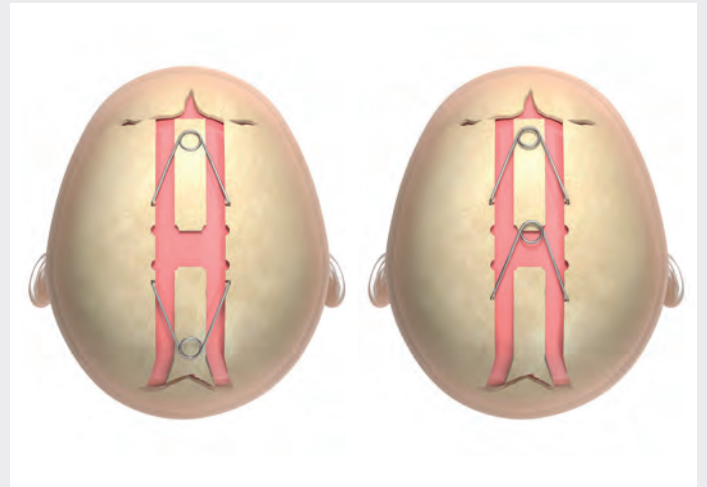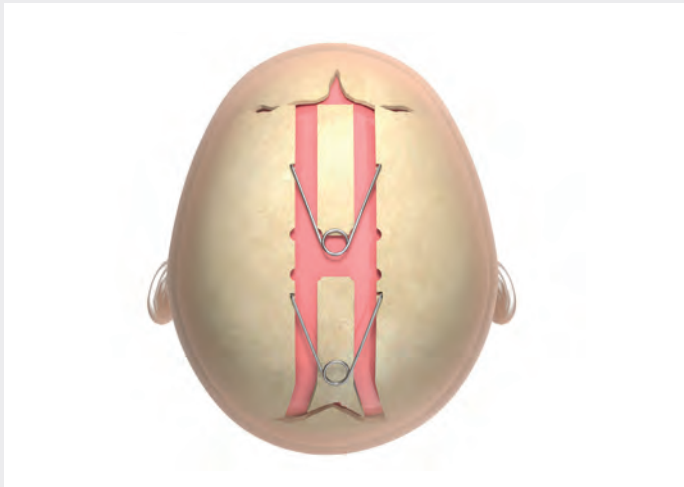

## 6. Determining the position of the spring

Typically, two springs are implanted.



The position of the springs is dictated by the characteristics of the case and adjusted to where the widening effect is required the most.

With a symmetrical scaphocephaly, the springs are placed in a standard fashion. This is typically 1 cm from the anterior and posterior to the cut bone square.

In the case of a particularly pinched anterior/posterior section, the springs may be placed more posteriorly or more anteriorly, to provide maximum vectoral force at the point where maximal expansion is required.

*Note:*

*For patient comfort, the placement of the posterior spring helix should avoid the occipital/resting area.*

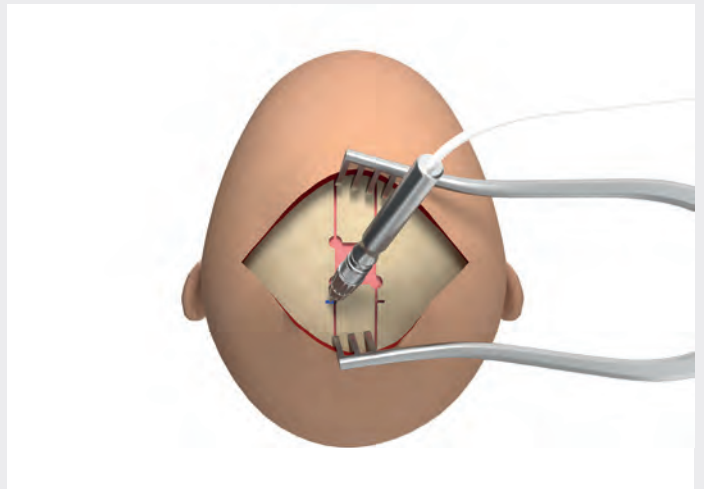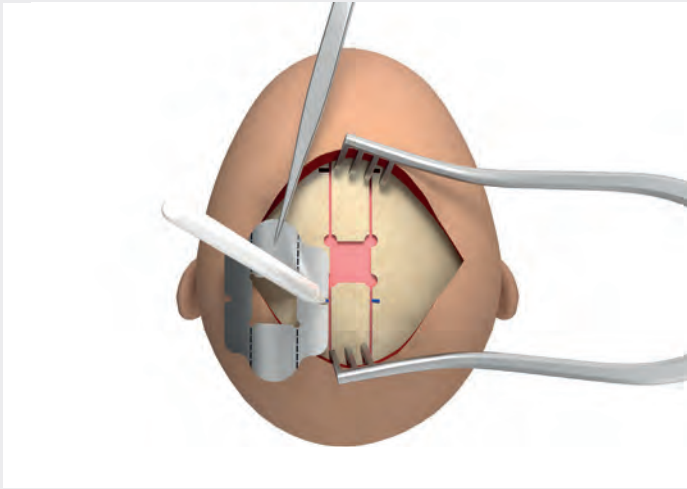

## 7. Preparation of implant bed/spring seat

Once the spring position has been determined, 2 mm deep slots are marked on the parietal bones perpendicular to the sagittal suture at the corresponding positions.

The springs have curved ends so that they sit firmly in these slots and ensure a secure hold.



Marking can be performed with the help of the marking template, which provides corresponding slots on the side.

The slots are created with the craniotome after marking.



Template for marking





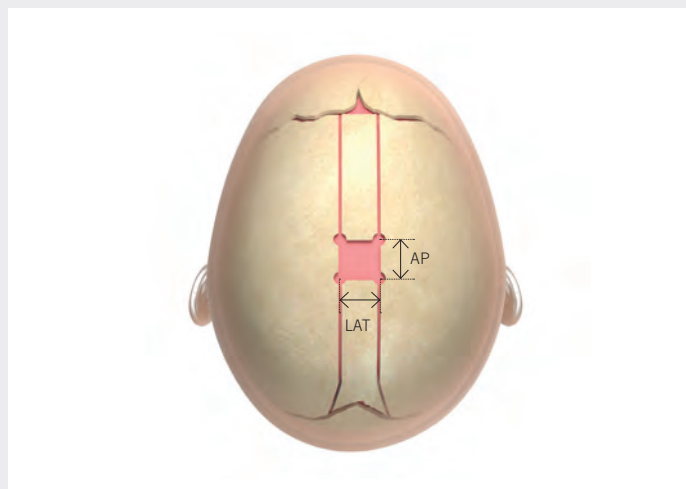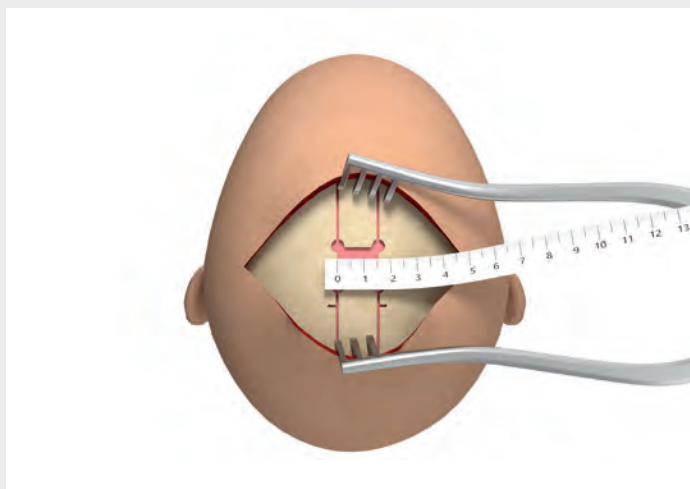

## 8. Measurements prior to spring insertion

Using a standard surgical ruler, the lateral edge-to-edge distance of the parietal bones (LAT) and the anterior-posterior distance (AP) of the craniotomy recess are measured before inserting the springs.

Measuring chart		
	Values after spring insertion	
<b>Lateral distance (LAT)</b> edge-to-edge distance of the parietal bones	_____ mm	
<b>Anterior-posterior distance (AP)</b> edge-to-edge distance of the craniotomy recess	_____ mm	

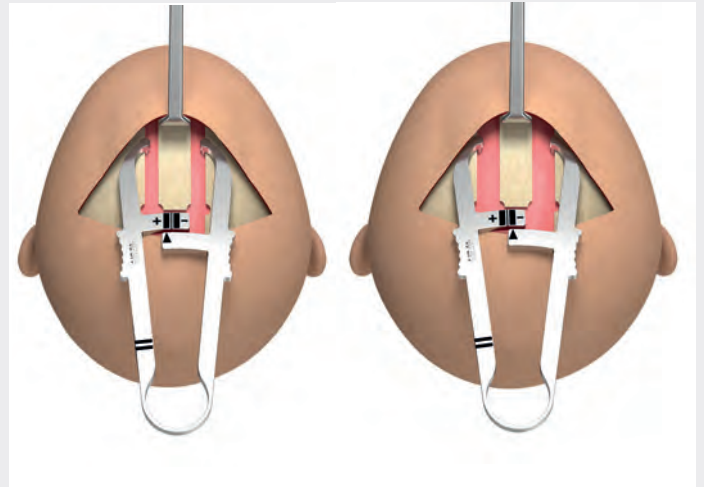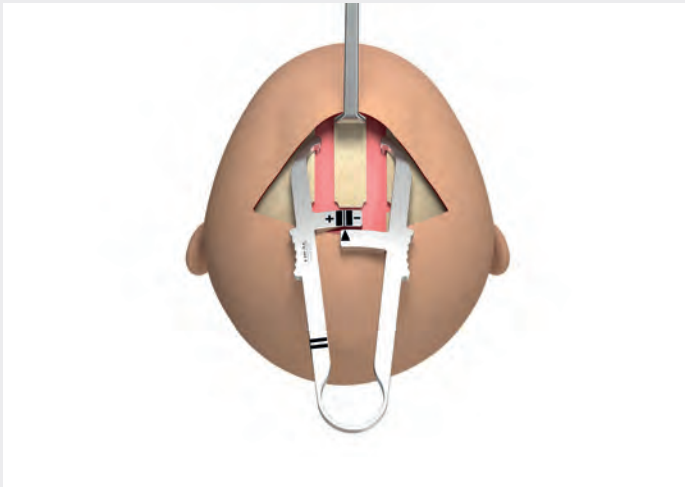

## 9. Selection of spring force (first spring)

The correct spring force is selected with the selection instrument. In terms of force, this is based on the medium, most commonly used spring with a spring thickness of  $\varnothing$  1.2 mm and is designed for an intraoperative expansion of the calvarium of 15 mm.

For measurement purposes, the selection instrument is hooked with its pins into the prepared slots to simulate implantation of the  $\varnothing$  1.2 mm spring.

If the arrow indicator is on the middle line, the spring with thickness 1.2 mm is the method of choice. If the arrow indicator lies to the right or to the left of the middle line, either a weaker (-) or a stronger (+) spring has to be chosen.

Finally, the overall opening from edge to edge of the parietal bones should be 30 mm (+/- 3 mm).

The arrow lies on the middle line:

Selection of  $\varnothing$  1.2 mm spring

The arrow lies to the left of the marked area (+):


Selection of  $\varnothing$  1.6 mm spring

The arrow lies to the right of the marked area (-):

Selection of  $\varnothing$  1.0 mm spring



Selection instrument

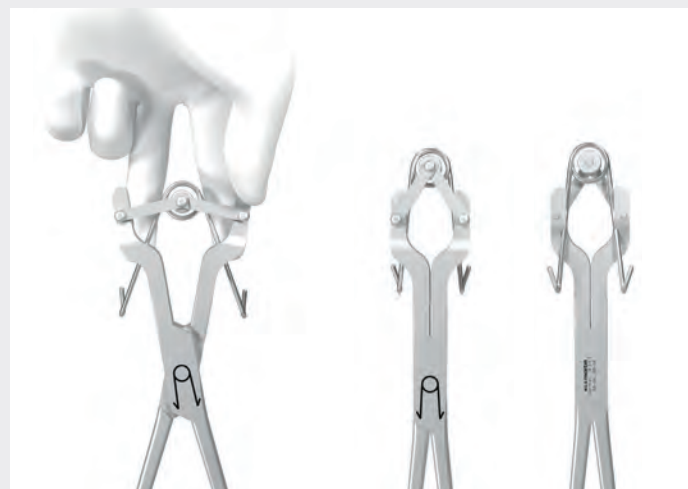

## 10. Pick-up of the spring with the insertion instrument

After determining the spring size, the spring is picked up with the corresponding insertion instrument.

Depending on the desired direction of insertion there are two instruments available:

### Spring opening to the front:

If the spring opening is to face to the front, the spring is picked up with insertion instrument 25-025-42-07. For this purpose, the spring helix is placed over the round coil of the instrument and the legs are inserted into the lateral guides when closing the instrument. This way, the spring ends are exposed and can be easily inserted into the prepared lateral slots.

### Spring opening to the rear:

If the spring opening is to face to the rear, the spring is picked up with insertion instrument 25-025-43-07. For this purpose, the spring helix is placed over the round coil of the instrument. The legs are placed into the lateral guides.


By closing the instrument with the locking mechanism, the spring is increasingly compressed and can be held in the desired position to enable easy insertion.



Insertion instrument




Insertion instrument

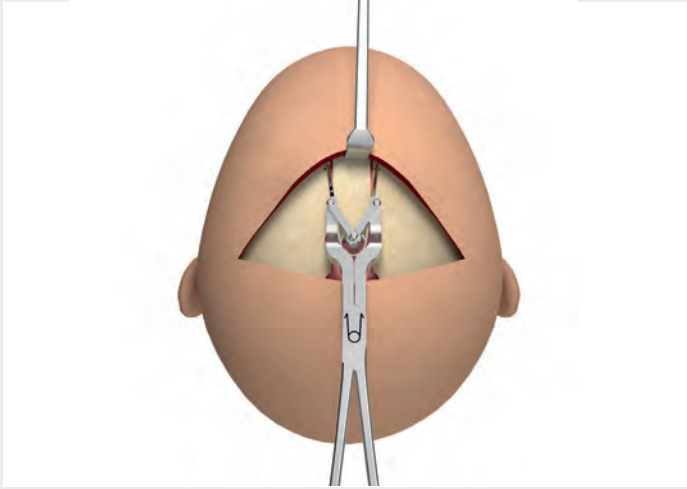


#### 11. Insertion of the first spring

The spring is inserted in such a way that the curved ends hook into the vertical slots. Once the spring is firmly seated and has a secure hold, the insertion instrument can be opened and removed.

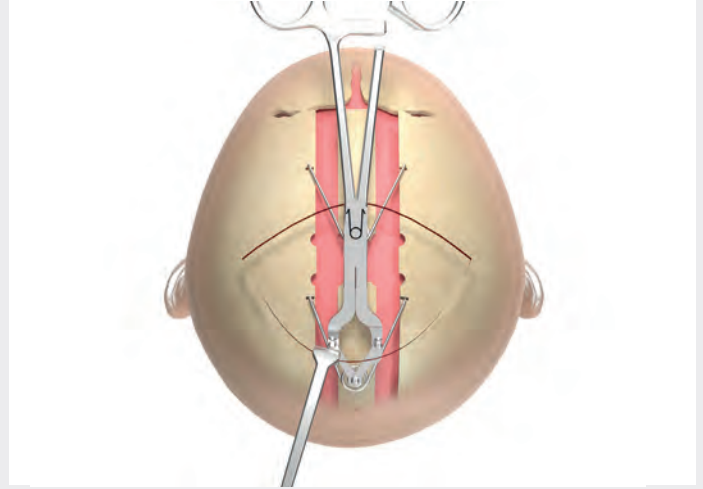

#### 12. Selection of spring force and insertion of the second spring



Selection of the spring thickness and insertion of the posterior spring is performed in the same manner as for the anterior spring. The procedure for this is described in steps 9 to 11.

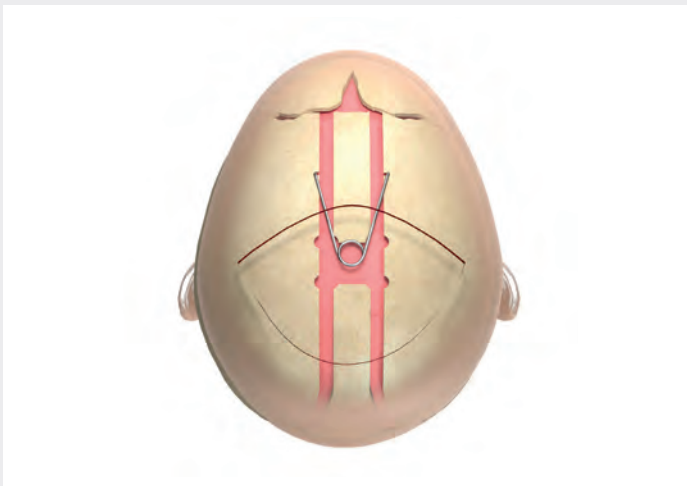

Selection instrument



Insertion instrument




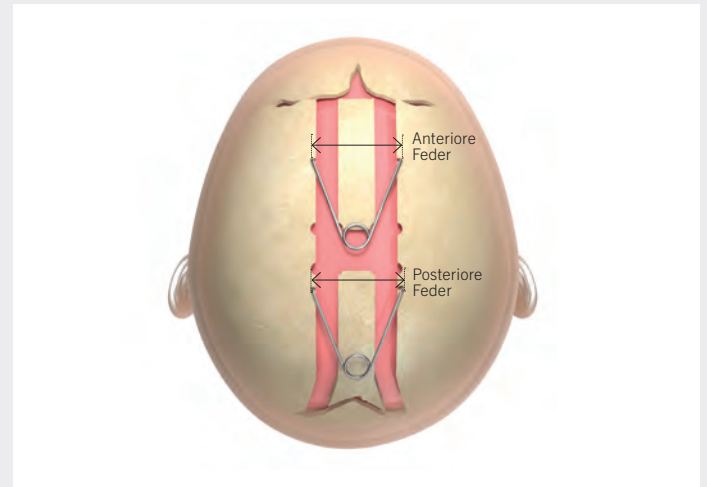
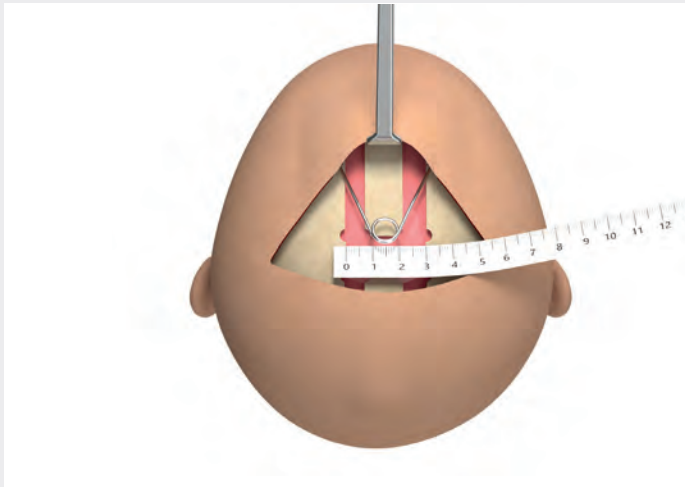


### 13. Measurements after spring insertion


After inserting the two springs, the edge-to-edge distance of the parietal bones (LAT) and the anterior-posterior distance (AP) of the craniotomy recess are measured.

Optionally, the overall opening of the legs at the curved ends can be measured for both springs.

To complete the dataset, we recommend measuring the distances between the two springs from each other (from the curved ends) as well as between the curved ends of the anterior spring and the coronal suture.

Measuring chart		
	Values after spring insertion	
<b>Lateral distance (LAT)</b> edge-to-edge distance of the parietal bones	_____ mm	
<b>Anterior-posterior distance (AP)</b> edge-to-edge distance of the craniotomy recess	_____ mm	
<b>Overall opening of the legs</b> from curved end to curved end	_____ mm	
Distance between the curved ends of the anterior spring and the coronal suture ( <b>A</b> )	_____ mm	
Distance between the springs to each other ( <b>B</b> ) from curved end to curved end	_____ mm	



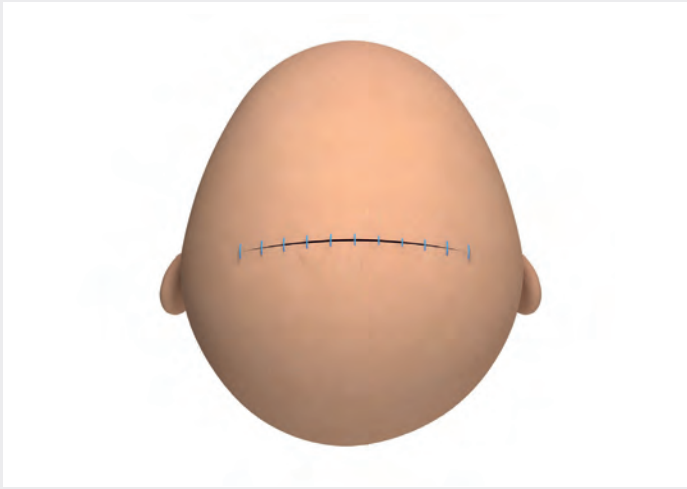

#### 14. Wound closure and postoperative treatment

Hemostasis during the procedure may require the use of Floseal, surgical measures and bone wax with electrocautery under direct vision. Once hemostasis is confirmed, a Betadine wash is used. Next, a 20 ml Redon drain is placed in situ, and a two-layered scalp closure is performed, typically using a 3-0 Vicryl for the galea and 4-0 Monocryl for the dermis.


This is followed by the application of a head bandage.

Twenty-four hours of intravenous antibiotics are given. Restrictions are not required.

The following day, the drain and the bandage are removed and X-rays of the skull are taken. The child can then generally be discharged.

Hair should not be washed until five days after the procedure.

CranioXpand springs are generally left in situ for 3 - 8 months.



## CranioXpand implants – springs in different wire thicknesses

### Cranial spring

Wire thickness Ø 1.0 mm



### Cranial spring

Wire thickness Ø 1.2 mm





Explanation of icons


**St** Stainless steel

**1** Packaging unit

**STERILE | R** Sterile packaged implants

### Cranial spring

Wire thickness Ø 1.6 mm

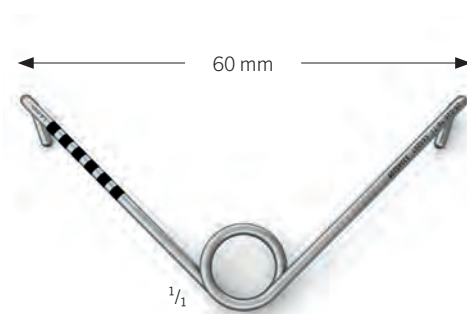

25-025-16-71

**STERILE | R**

**St 1**


## CranioXpand instruments – standard instrumentation



½

25-025-40-07  
Template for marking

St 1

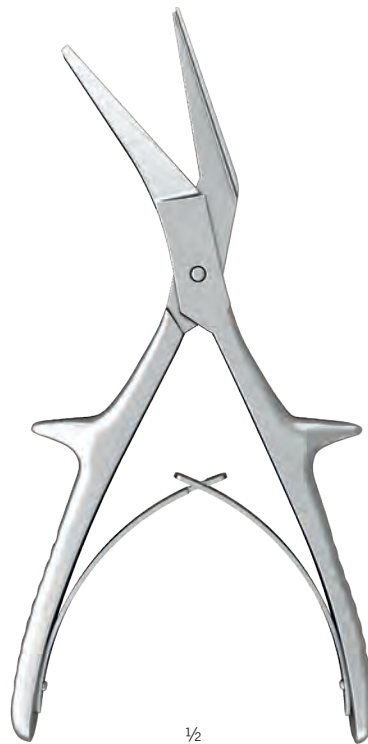

½

48-297-19-07  
Bone cutting forceps

St 1



½

25-025-52-07  
Selection instrument

St 1





Explanation of icons

- St** Stainless steel
- 1** Packaging unit



1/2

25-025-42-07  
Insertion instrument  
Spring opening to the front

**St 1**



1/2

25-025-43-07  
Insertion instrument  
Spring opening to the rear


**St 1**



1/2

25-025-45-07  
Instrument for lifting springs

**St 1**

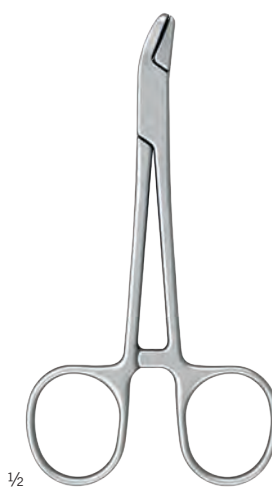

1/2

25-025-44-07  
Instrument for removing springs

**St 1**

## Storage **CranioXpand** for standard instrumentation

The storage system is not only simple and well-designed, for example with the instruments arranged according to their sequence of use during surgery, it also ensures optimum reprocessing due to large openings in the honeycomb design to equally serve the needs of all involved parties.

All the instruments required for an operation can be stored individually next to each other in the storage container.


The individual storage locations are marked with a laser on the base with an article number and illustration, making it easier to sort the instruments after cleaning.



<b>55-925-10-04</b>	<b>CranioXpand Instrument storage container set, comprised of:</b>
55-925-11-04	Instrument container
55-910-59-04	Lid



55-925-11-04  
Instrument container



55-910-59-04  
Lid

## KLS Martin Group

### **KLS Martin Australia Pty Ltd.**

Sydney · Australia  
Tel. +61 2 9439 5316  
australia@klsmartin.com

### **KLS Martin do Brasil Ltda.**

São Paulo · Brazil  
Tel. +55 11 3554 2299  
brazil@klsmartin.com

### **KLS Martin Medical (Shanghai) International Trading Co., Ltd**

Shanghai · China  
Tel. +86 21 5820 6251  
info@klsmartin.com

### **KLS Martin India Pvt Ltd.**

Chennai · India  
Tel. +91 44 66 442 300  
india@klsmartin.com

### **KLS Martin Italia S.r.l.**

Milan · Italy  
Tel. +39 039 605 67 31  
info@klsmartin.com

### **KLS Martin Japan K.K.**

Tokyo · Japan  
Tel. +81 3 6410 8471  
japan@klsmartin.com

### **KLS Martin SE Asia Sdn. Bhd.**

Penang · Malaysia  
Tel. +604 261 7060  
malaysia@klsmartin.com

### **KLS Martin de México, S.A. de C.V.**

Mexico City · Mexico  
Tel. +52 55 7572 0944  
mexico@klsmartin.com

### **KLS Martin Nederland B.V.**

Huizen · Netherlands  
Tel. +31 35 523 45 38  
info@klsmartin.com

### **KLS Martin SE & Co. KG**

Moscow · Russia  
Tel. +7 499 792 76 19  
russia@klsmartin.com

### **KLS Martin Taiwan Ltd.**

Taipei · Taiwan  
Tel. +886 2 2325 3169  
taiwan@klsmartin.com

### **KLS Martin SE & Co. KG**

Dubai · United Arab Emirates  
Tel. +971 4 454 16 55  
middleeast@klsmartin.com

### **KLS Martin UK Ltd.**

Reading · United Kingdom  
Tel. +44 118 467 1500  
info.uk@klsmartin.com

### **KLS Martin LP**

Jacksonville · Florida, USA  
Tel. +1 904 641 77 46  
usa@klsmartin.com

### **KLS Martin SE Asia Sdn. Bhd.**

Hanoi · Vietnam  
Tel. +49 7461 706-0  
vietnam@klsmartin.com



### **KLS Martin SE & Co. KG**

#### **A company of the KLS Martin Group**

KLS Martin Platz 1 · 78532 Tuttlingen · Germany  
PO Box 60 · 78501 Tuttlingen · Germany  
Tel. +49 7461 706-0 · Fax +49 7461 706-193  
info@klsmartin.com · www.klsmartin.com